

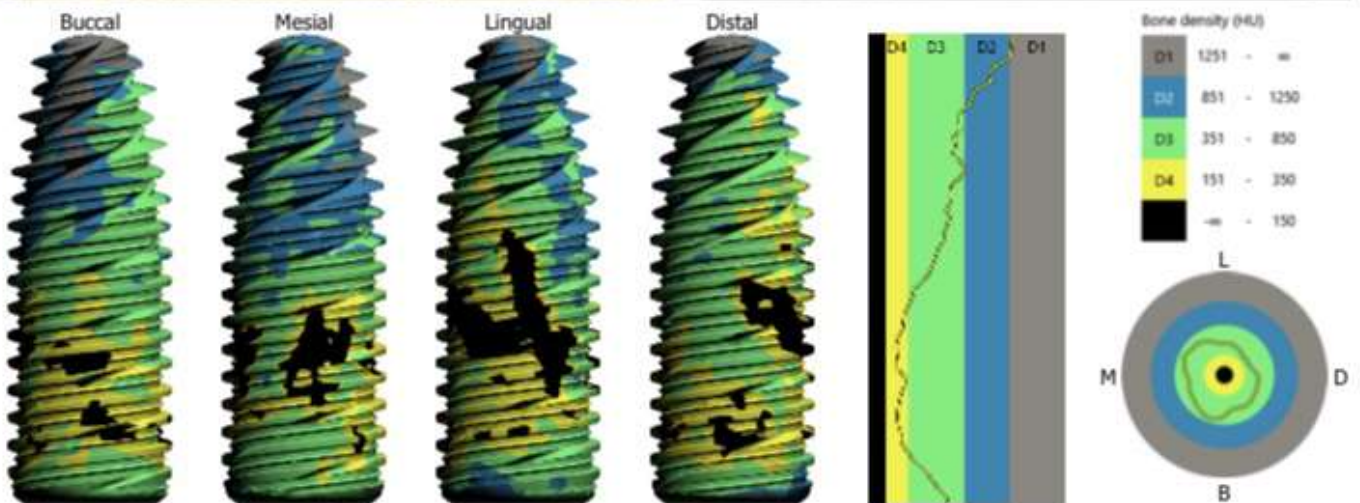
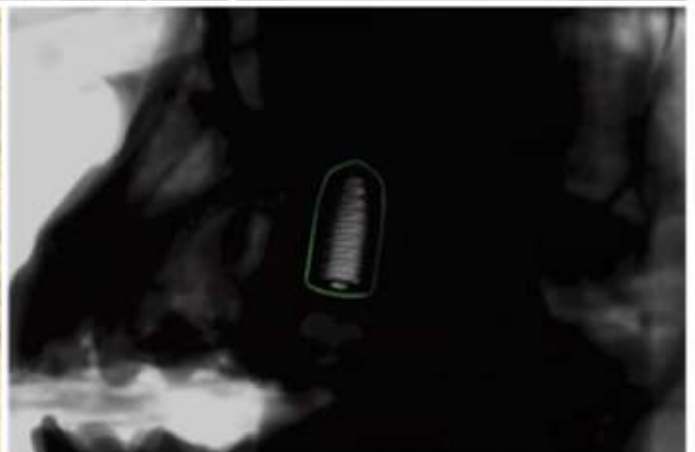
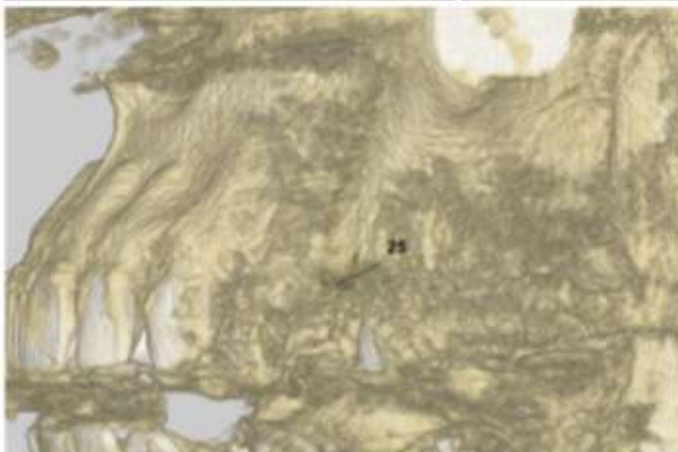
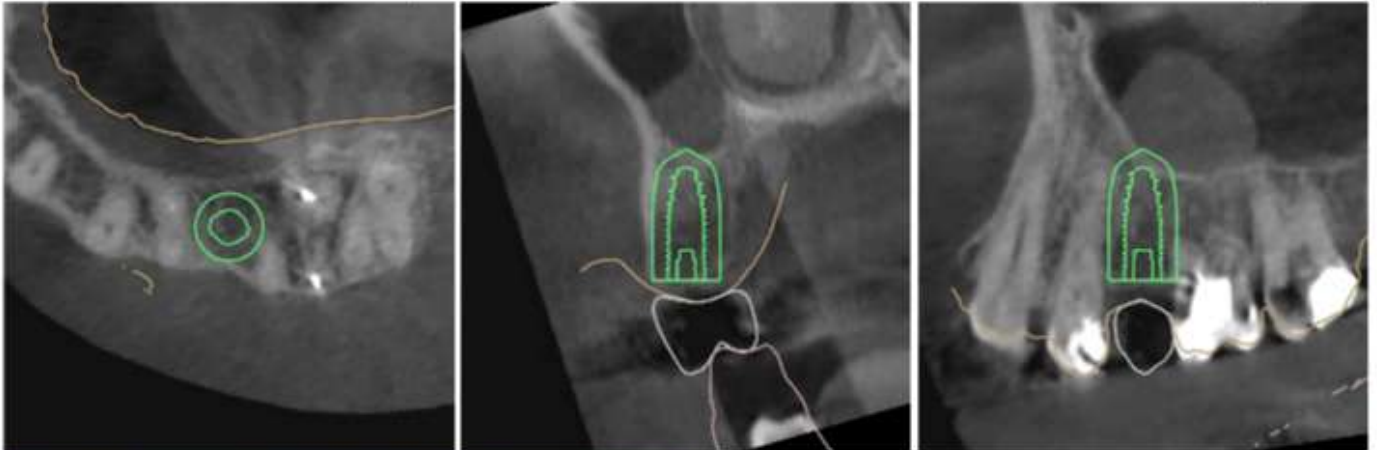


Implant Information		
Implant position (FDI)	25	
Manufacturer	Biotech Dental	
Type	Biotech Dental KONTACT Internal 4.2x12.0	
Order number	K4212	
Length, mm	12	
Diameter (Ø), mm	4.2	
Color	Blue 	
Safety zone - apical distance	2.0	
Safety zone - radial distance	1.5	



Limitation of Liability:

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.